



# VirtualFLOW™100

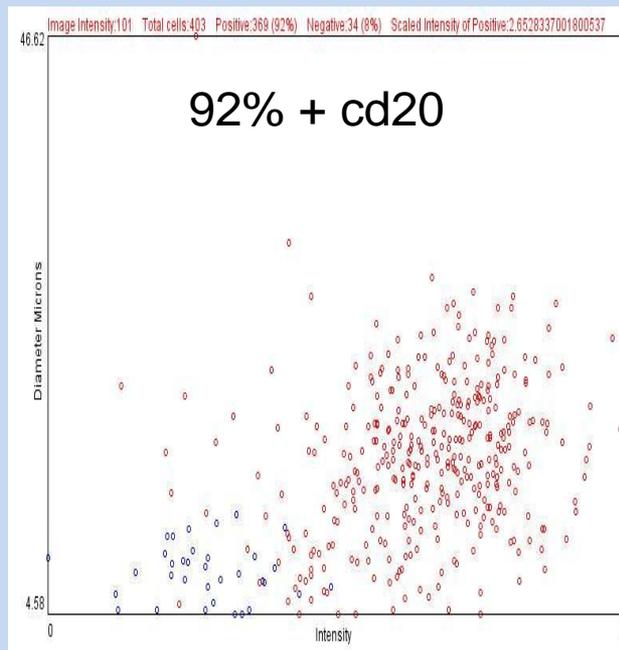

For Cd20 and most strong diffuse staining cell markers

Converts a strongly back-to-back positive immunostained tissue section to a digital form with calculated positive percentage result using microscope images

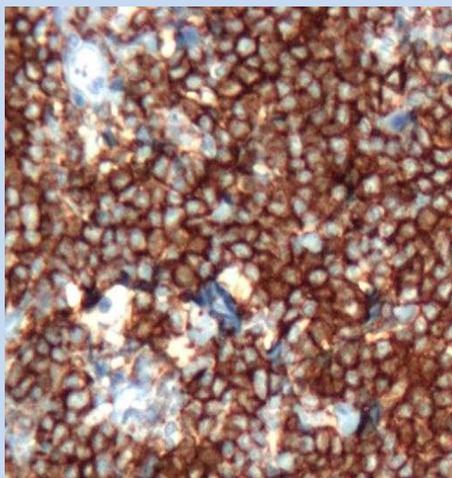